

Fig. 1

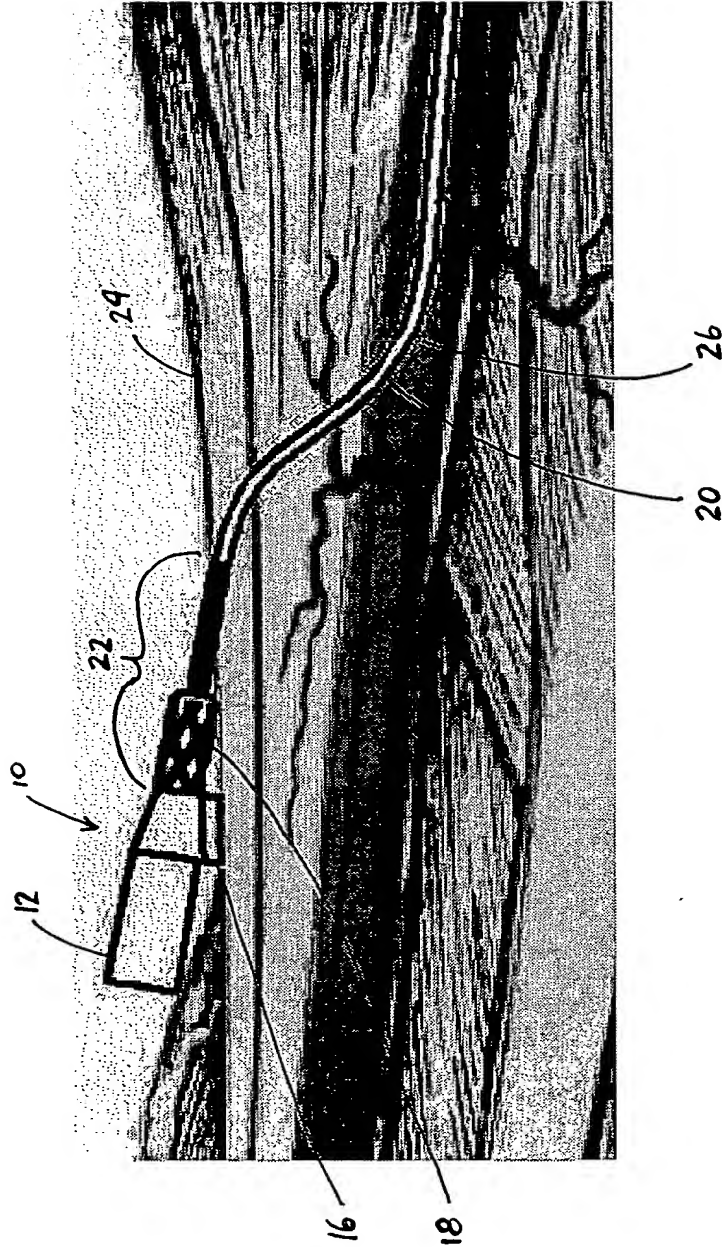


Fig. 2

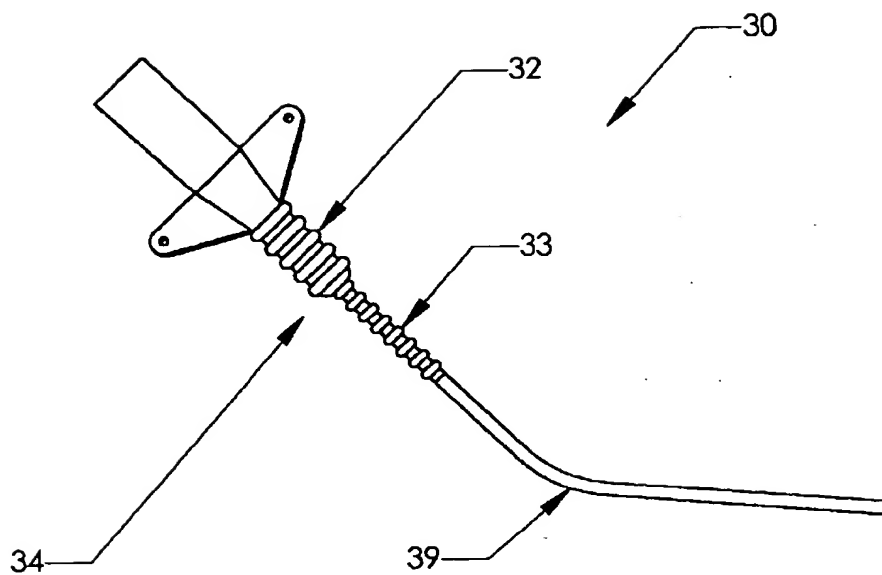


Fig. 3

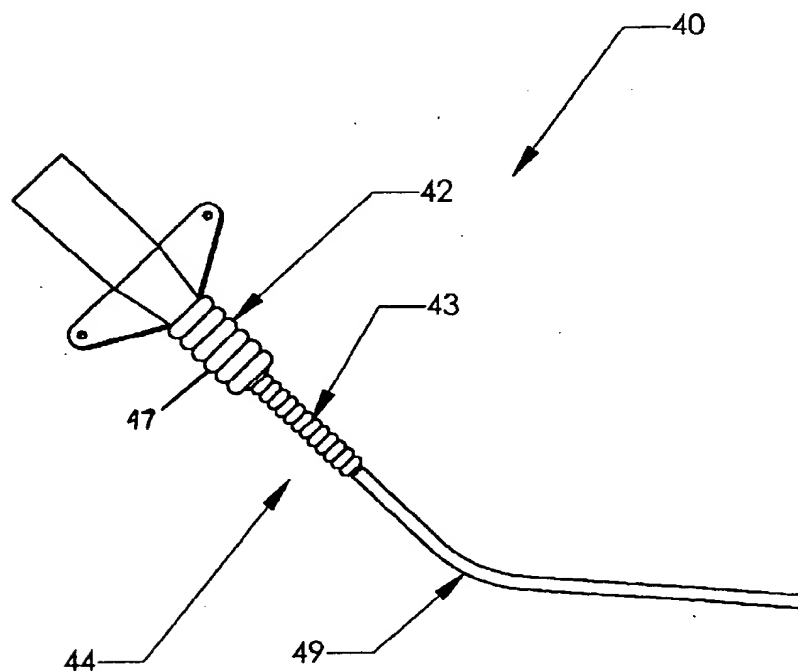


Fig. 4

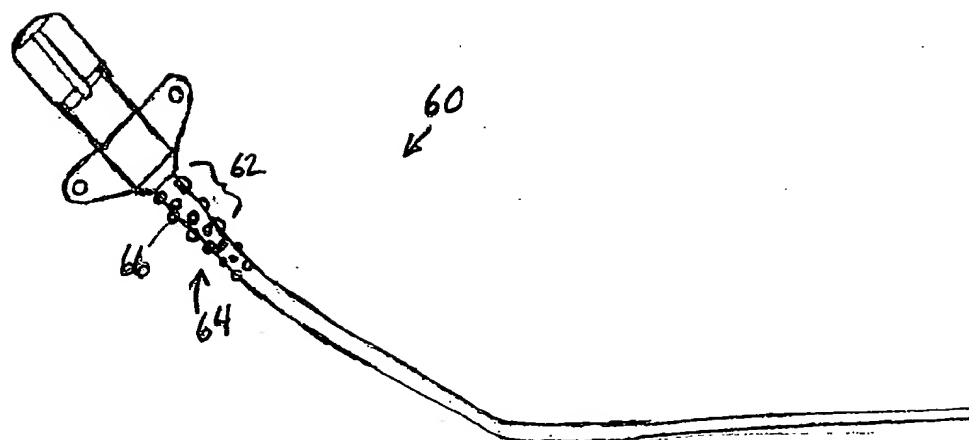
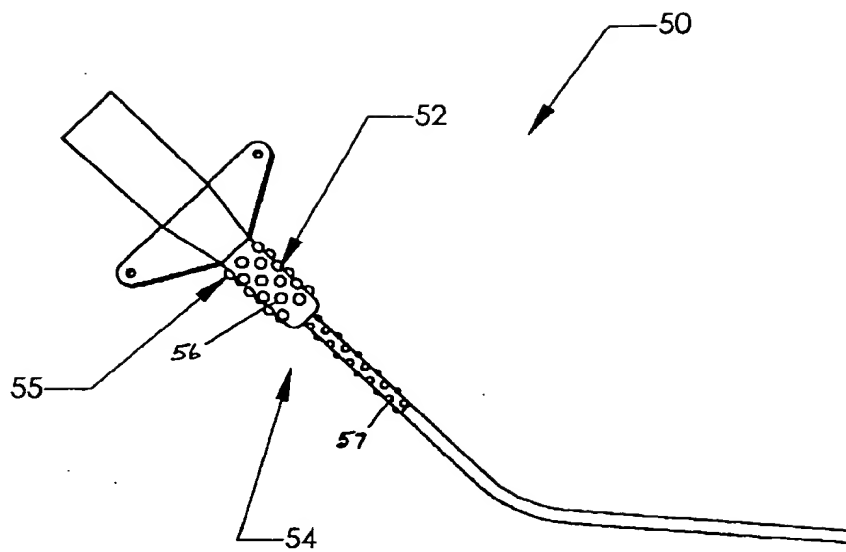


FIG. 7 is a perspective view of the device in a second position, with the handle 78 and the shaft 76 in a retracted position, and the probe 70 in an extended position.

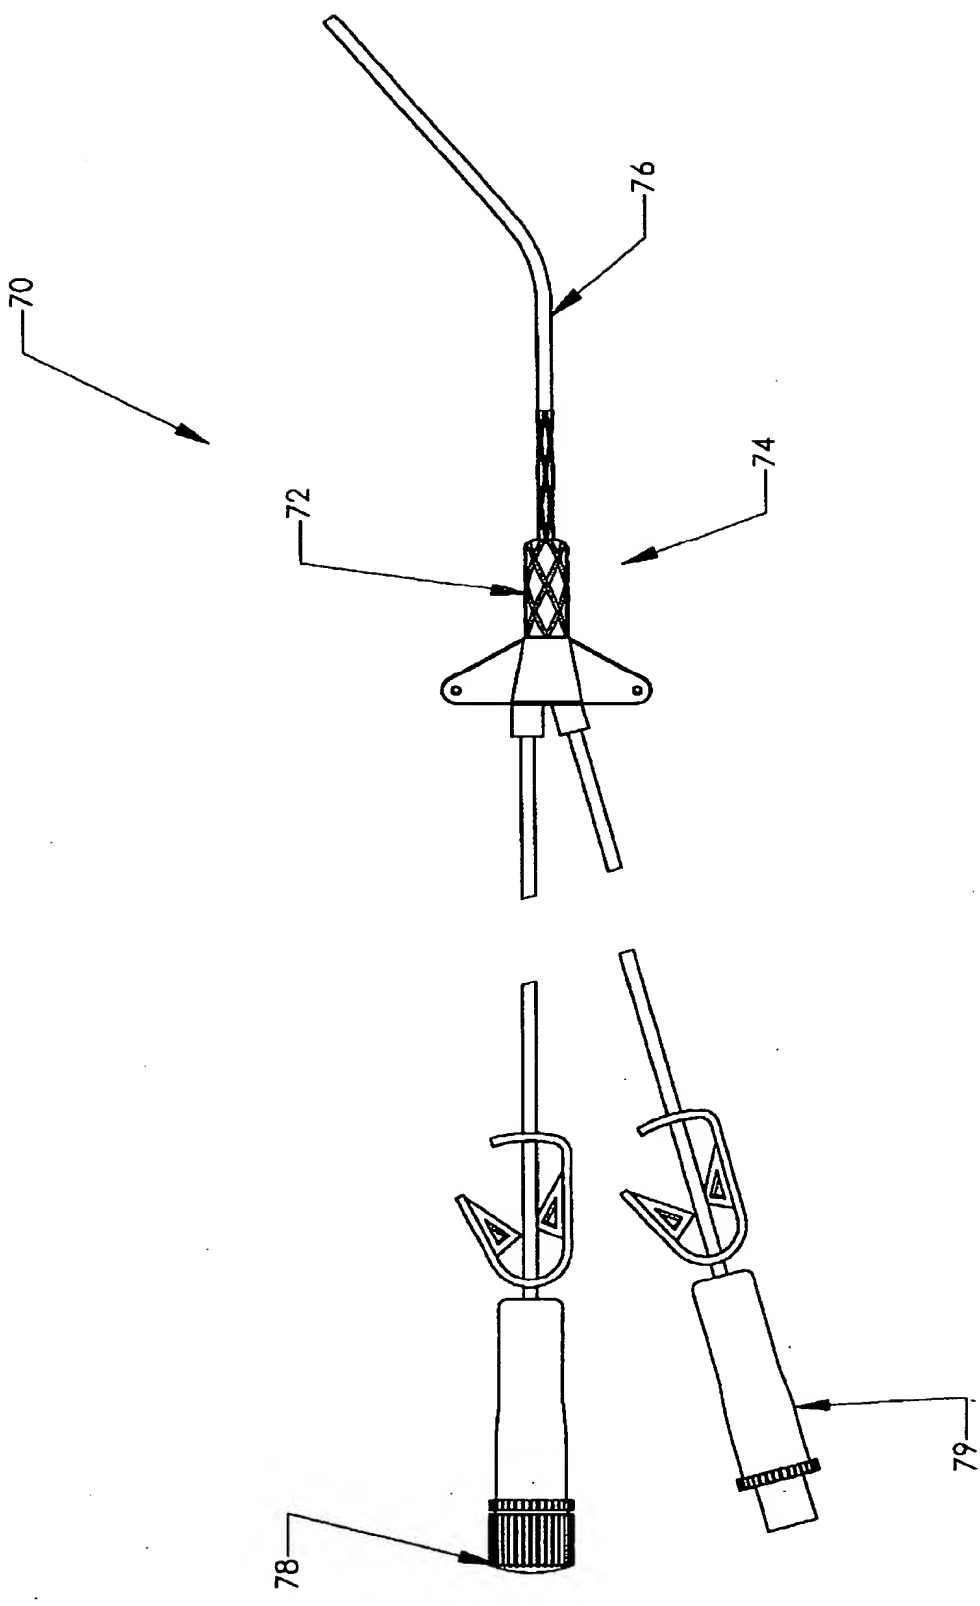


Fig. 7

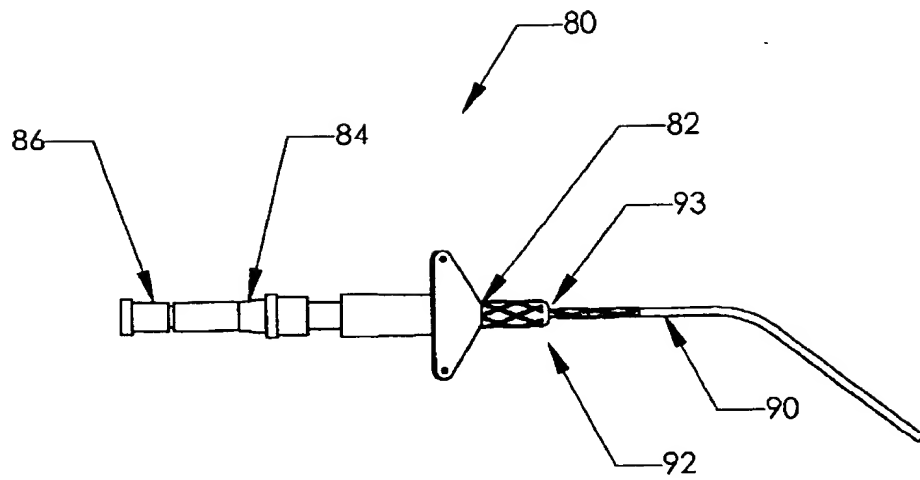


Fig. 8

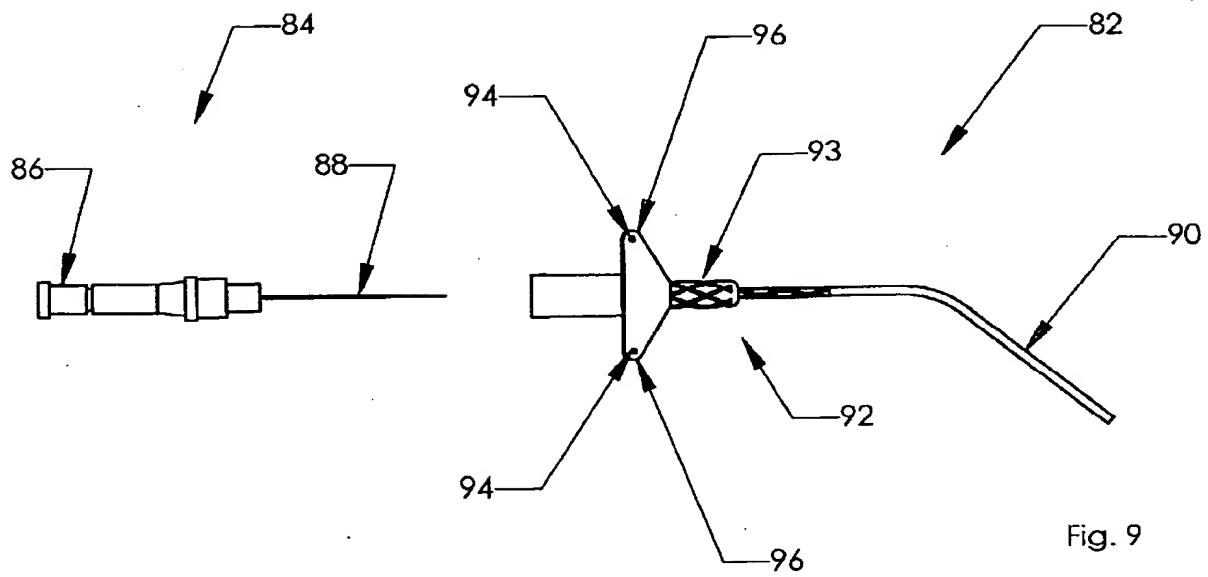


Fig. 9

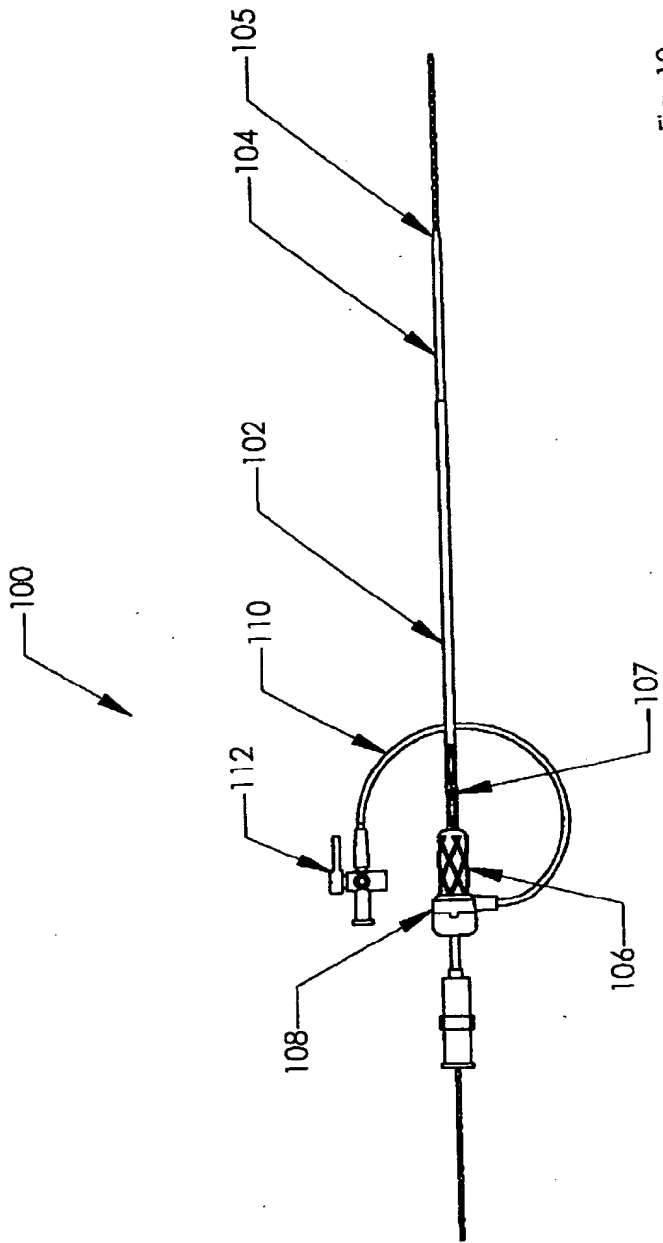


Fig. 10

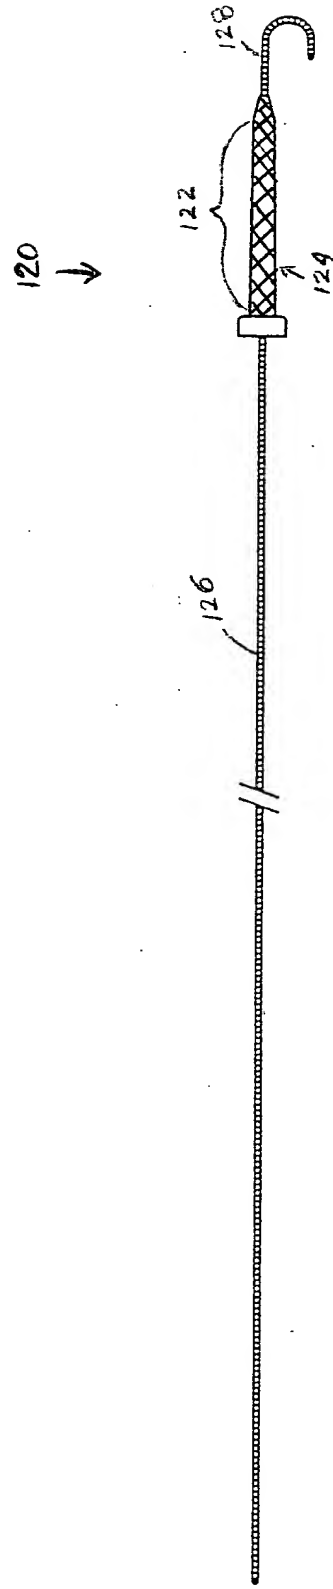


FIG 11

05172573 040100